



# CHI150 Saturated Calomel Electrode (SCE)

## Introduction



$E^0 = 0.241\text{V}$  vs NHE at  $25^\circ\text{C}$  for saturated calomel electrode (SCE)

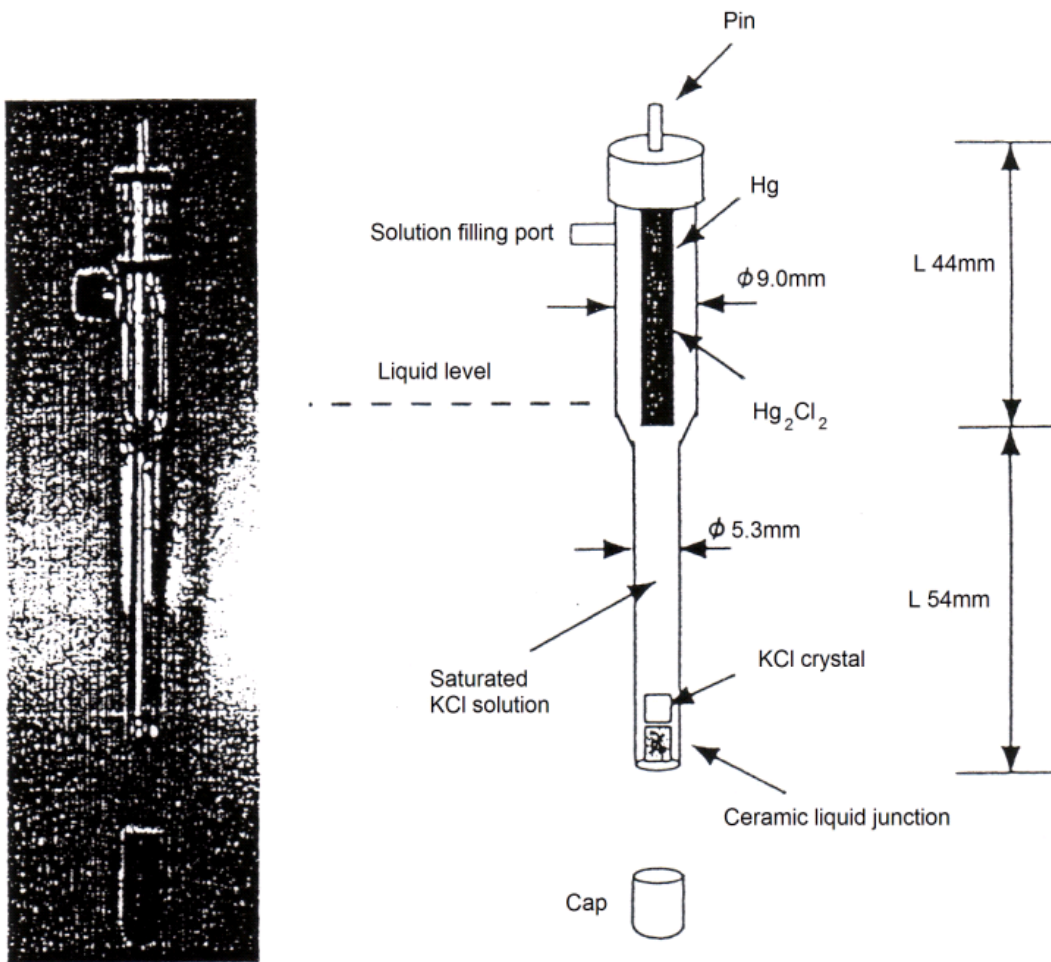

## Note:

1. Please remove cap before first time use.
2. If there is air bubbles trapped in the chamber, please swing the electrode body to remove air bubbles.
3. If the solution inside the electrode is below the liquid level shown above, please fill saturated  $\text{K}_2\text{Cl}_2$  solution.
4. After use, please dip the electrode into saturated  $\text{K}_2\text{Cl}_2$  solution.

CH Instruments, Inc.  
3700 Tennon Hill Drive  
Austin, TX 78738 USA  
Tel: (512) 402-0176 Fax: (512) 402-0186  
E-mail: info@chinstruments.com